

This Page Is Inserted by IFW Operations
and is not a part of the Official Record

BEST AVAILABLE IMAGES


Defective images within this document are accurate representations of the original documents submitted by the applicant.

Defects in the images may include (but are not limited to):

- BLACK BORDERS
- TEXT CUT OFF AT TOP, BOTTOM OR SIDES
- FADED TEXT
- ILLEGIBLE TEXT
- SKEWED/SLANTED IMAGES
- COLORED PHOTOS
- BLACK OR VERY BLACK AND WHITE DARK PHOTOS
- GRAY SCALE DOCUMENTS

IMAGES ARE BEST AVAILABLE COPY.

**As rescanning documents *will not* correct images,
please do not report the images to the
Image Problem Mailbox.**



Before Pre-hyb

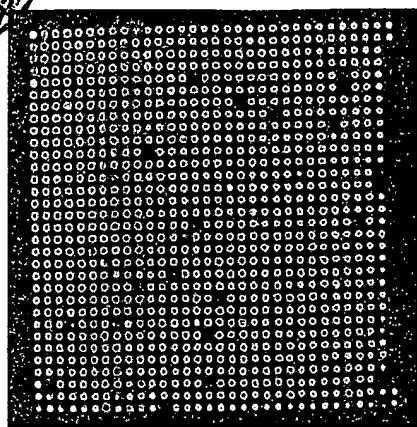


Fig. 1A

Post pre-hybe w/o NaBH4

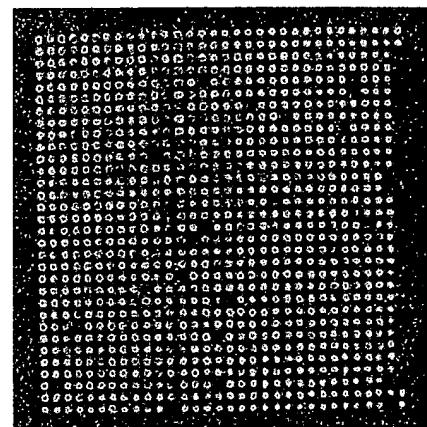


Fig. 1B

Post pre-hybe w/ NaBH4

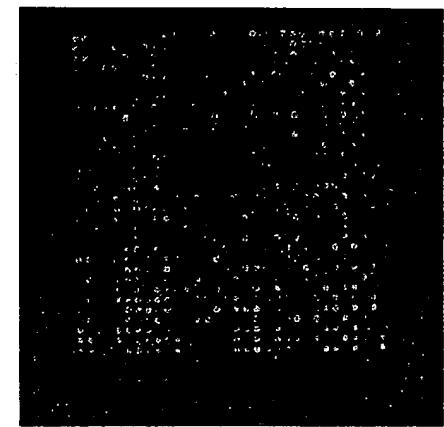


Fig. 1C

**Autofluorescence reduction using NaBH4
on Human 6K array**

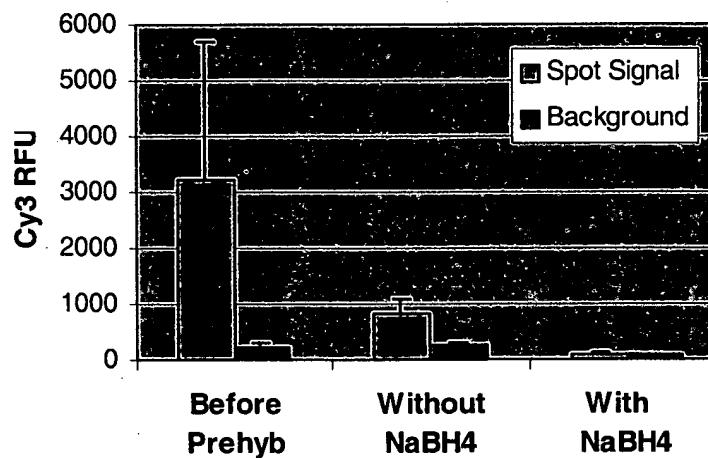


Fig. 2

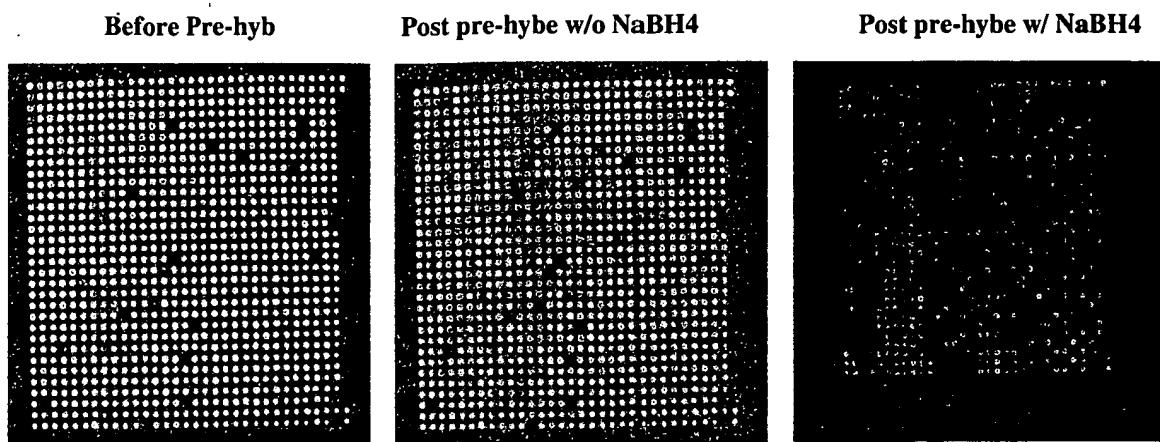


Fig. 3A

Fig. 3B

Fig. 3C



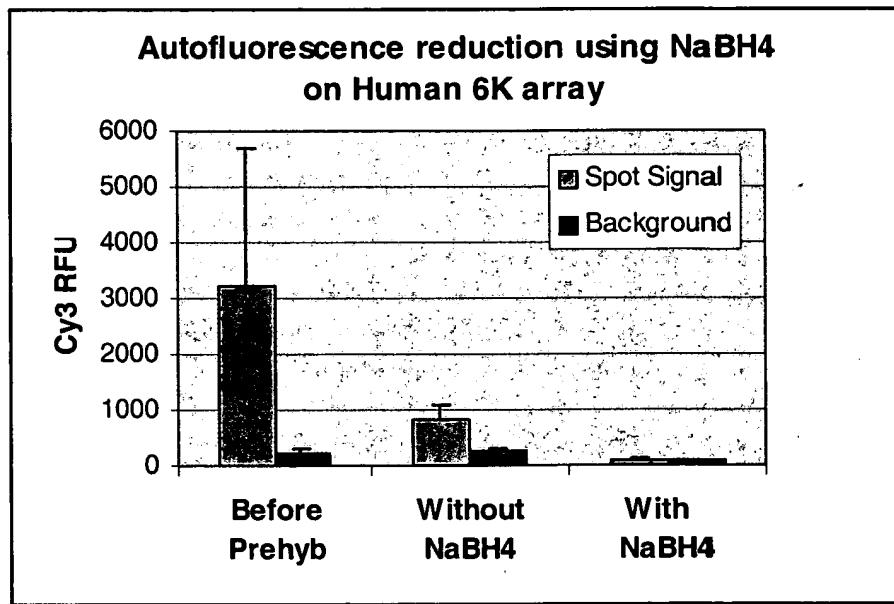


Fig. 4

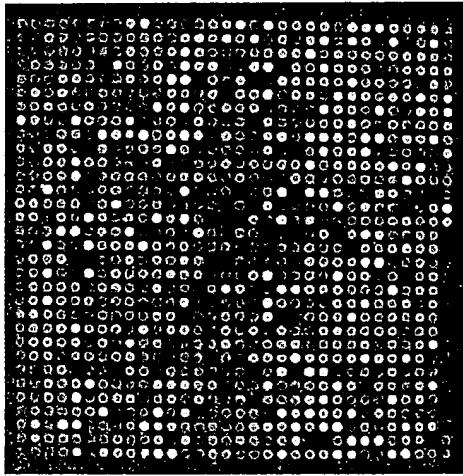

Without NaBH4 Treatment

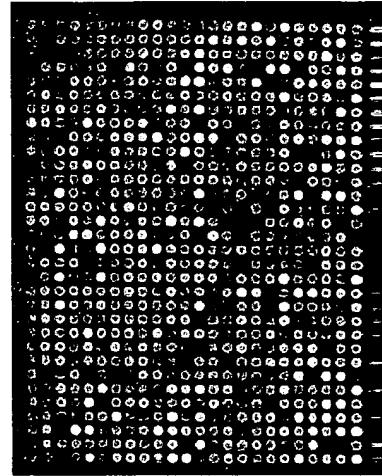

With NaBH4 Treatment

Fig. 5A

Fig. 5B

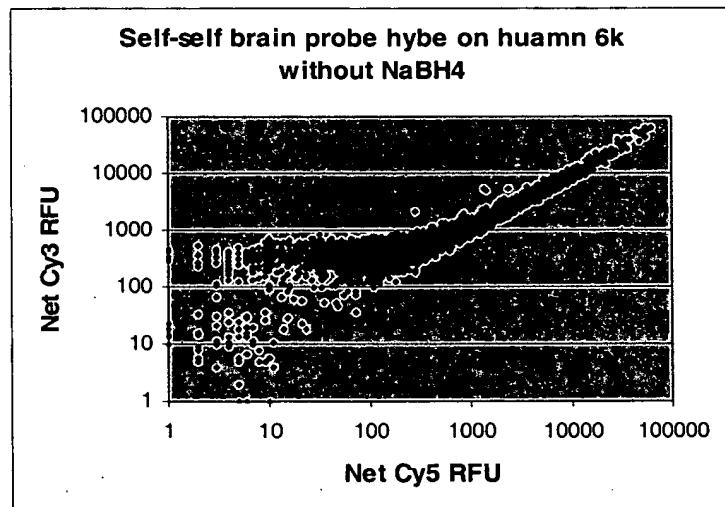


Fig. 6A

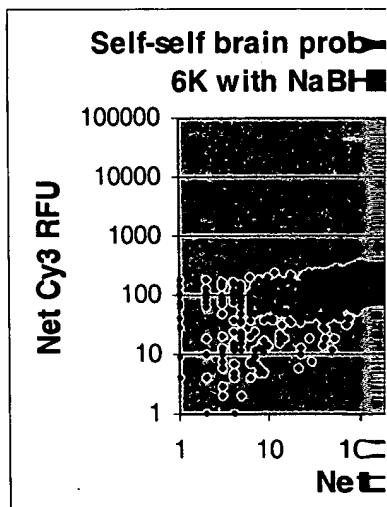


Fig. 6B




Fig. 7A



Fig. 7B




Fig. 7C




Fig. 7D

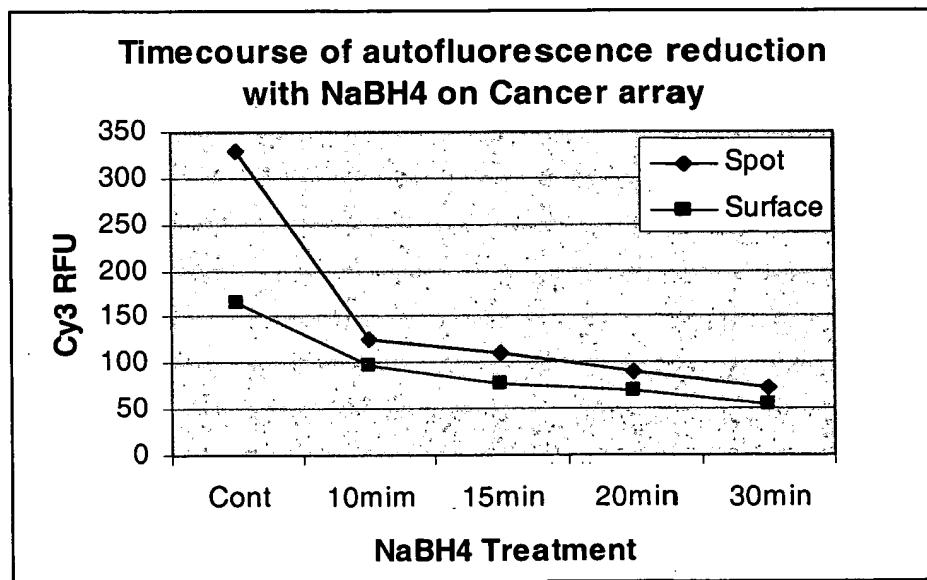


Fig. 8

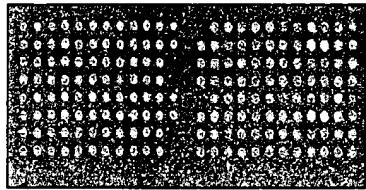


Fig. 9A

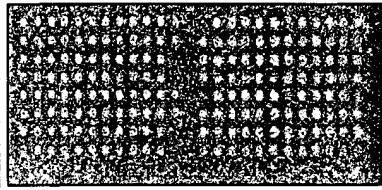


Fig. 9B

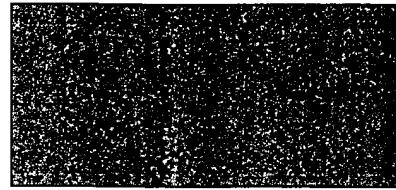


Fig. 9C




Fig 10A




Fig. 10B




Fig. 10C

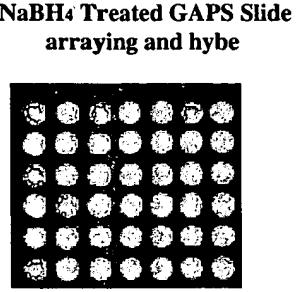


Fig. 10D

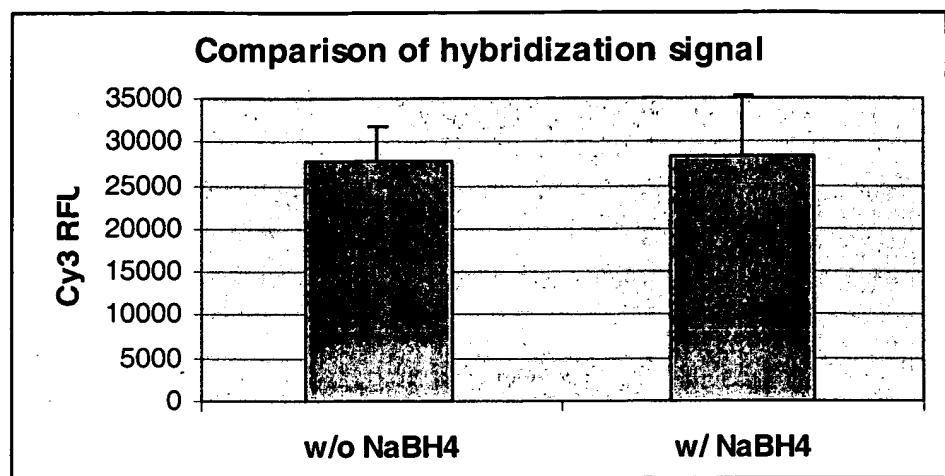


Fig. 11A

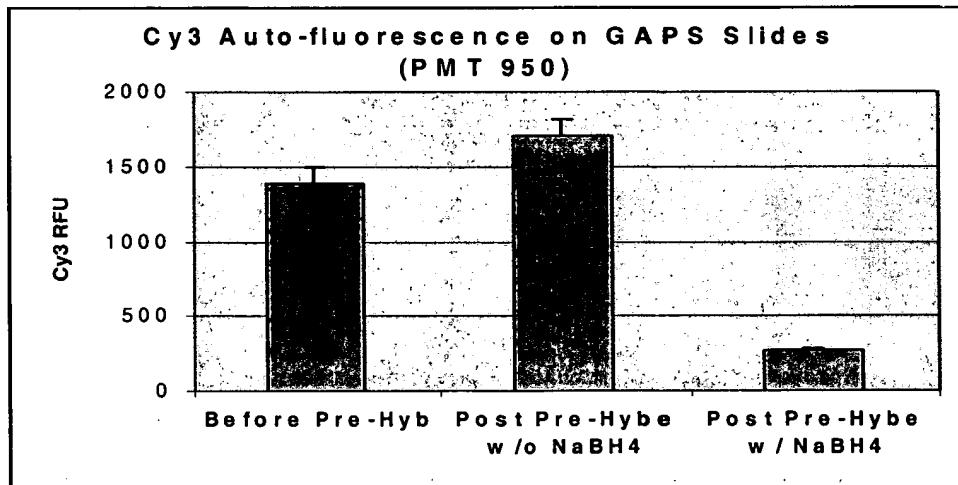


Fig. 11B